



EU Type Examination Certificate Number: 0120/SGS0083/R1

EM-Lite Limited

1 Stevern Way
Peterborough
Cambridgeshire
PE1 5EL

Instrument Identification:
ECA1.*, EMA1.*, EMB1.*, EMC1.*

Single Phase, Credit, Active Import/ Export, Modular, Electricity Meter

Instrument Traceable Number
0120/SGS0083

has been assessed and certified as meeting the requirements of

EU Directive 2014/32/EU
on Measuring Instruments Annex II, Module B

It is certified that the manufacturer's technical design and specimen for the above instrument has been examined and, based on the evidence submitted, it is considered that the instrument conforms to the requirements of Annex V of EU Directive 2014/32/EU

This certificate must be used in conjunction with a certificate covering the product verification as required in Annex II, Module D or Annex II, Module F

This certificate is valid until 22nd March 2030

Issue 2

Certification is based on report number(s) EMA146218 dated 24th May 2011, EMA149885 dated 12th August 2011
EMA155457 dated 17th January 2012, EMA190713 dated 23rd January 2015, EMA277441 dated 23rd March 2022

Authorised Signature

Tuomas Hänninen

SGS Fimko OY, Notified Body 0598
Takomatie 8, FI-00380 Helsinki, Finland
t +358 9 6963 61 www.sgs.fi



	EU-Type Examination Certificate Number:	
	0120/SGS0083/R1	
	Issue Number: 2	Dated: 19 th June 2024

1. Technical Data

Manufacturer	EM-Lite Ltd
Meter Type(s)	ECA1.*, EMA1.*, EMB1.*, EMC1.*
Voltage Rating (U_n)	220-240V
Current Rating ($I_{min} - I_{ref} (I_{max})$)	0,25-5(100)A 0,5-10(100)A 0,75-15(100)A 1-20(100)A
Frequency (F_n)	50Hz
Active Accuracy Class (kWh)	A or B (kWh)
Type of circuit	1p2w
Temperature Range	-40°C to +70°C
Software/ Firmware Version No's	See list overleaf
CRC Checksum	See list overleaf
Identification Location	LCD
Bill of Materials No's	See list overleaf
IP Rating	IP52
Insulation Protective Class	Class II
LED Pulse Constant	1000 imp/ kWh
Impulse Voltage Rating	8kV
AC Voltage Rating	4kV
Main Cover Sealing Type	Wire & Crimp x 1
Integrity of meter	Inaccessible without breaking seals
Intended Location of the Meter	Indoor
Type of Register	LCD
Terminal Arrangement(s)	BS
Location of Manufacturers Address	Nameplate



EU-Type Examination Certificate Number:

0120/SGS0083/R1

Issue Number: 2

Dated: 19th June 2024**Bill of Materials****Meter Variant****BOM Number**

EMA1.z
EMA1.az
EMA1.y
EMA1.ay
EMA1.x
EMA1.w

EMA1-4002-04
EMA1-4003-08
EMA1-4001-08
EMA1-4004-04
EMA1-4002-04
EMA1-4001-08

EMB1.z
EMB1.y
EMB1.ay
EMB1.x
EMB1.w

EMB1-4002-04
EMB1-4001-08
EMB1-4003-05
EMB1-4002-04
EMB1-4001-08

EMC1.z
EMC1.az
EMC1.y
EMC1.ay
EMC1.x
EMC1.w
EMC1.by
EMC1.cz

EMC1-4002-04
EMC1-4003-04
EMC1-4001-07
EMC1-4004-03
EMC1-4002-04
EMC1-4001-07
EMC1-4005-03
EMC1-4007-05



EU-Type Examination Certificate Number:

0120/SGS0083/R1

Issue Number: 2

Dated: 19th June 2024

Software Version Numbers

EMA1, EMB1, ECA1

V3.00-1
V3.02-0
V3.03-2
V3.04-0 Checksum 32995
V3.20-1 Checksum 61849
V3.20-2 Checksum 64953
V3.20-4 Checksum 60932

EMA1.y or .z, EMB1.y or .z

V3.10-0 Checksum 39352
V3.11-1 Checksum 16259
V3.11-2 Checksum 08820
V3.20-1 Checksum 61849
V3.20-2 Checksum 64953
V3.20-4 Checksum 60932

EMC1.*

V0.00-3
V1.00-0
V1.01-3
V1.02-0 Checksum 10305
V1.02-1 Checksum 22571
V2.00-1 Checksum 49889
V2.00-3 Checksum 40683
V3.00-0 Checksum 18714
V3.00-3 Checksum 25532
V3.10-1 Checksum 42711

EMC1.cz

V3.80-4 Checksum 19684

SGS

EU-Type Examination Certificate Number:


0120/SGS0083/R1

Issue Number: 2


Dated: 19th June 2024

2. Photographs of Meter and Sealing Plan

EM*1 with MC11 Module Fitted

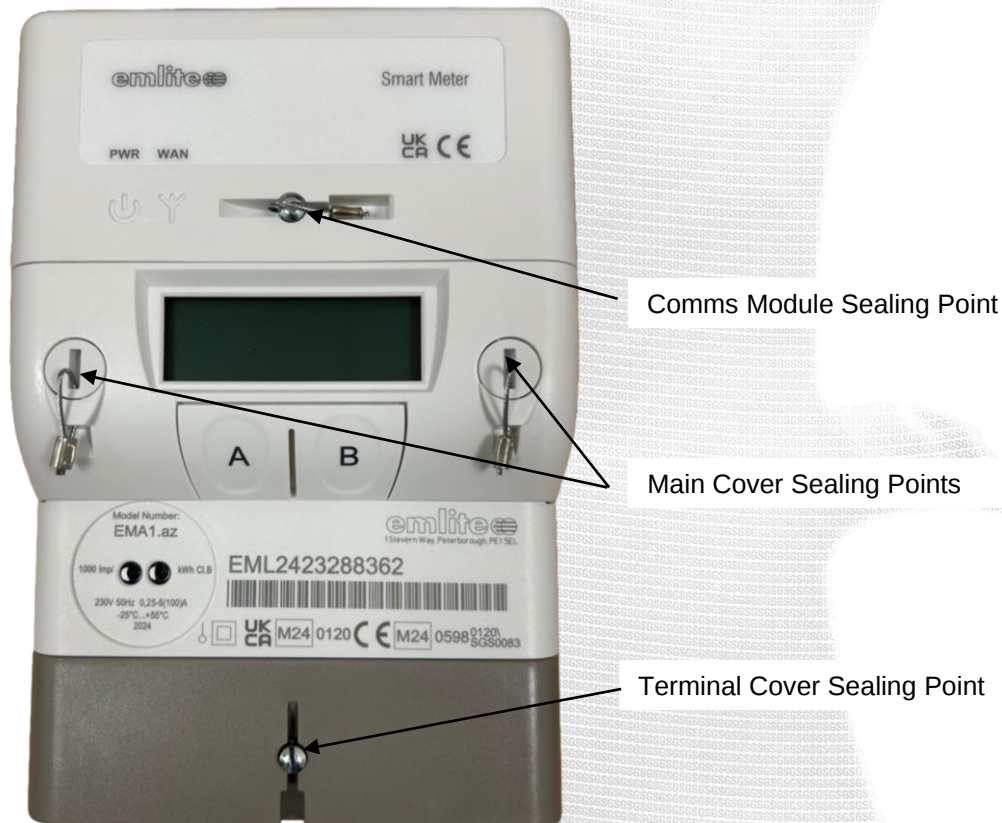

EM*1 No Module Fitted

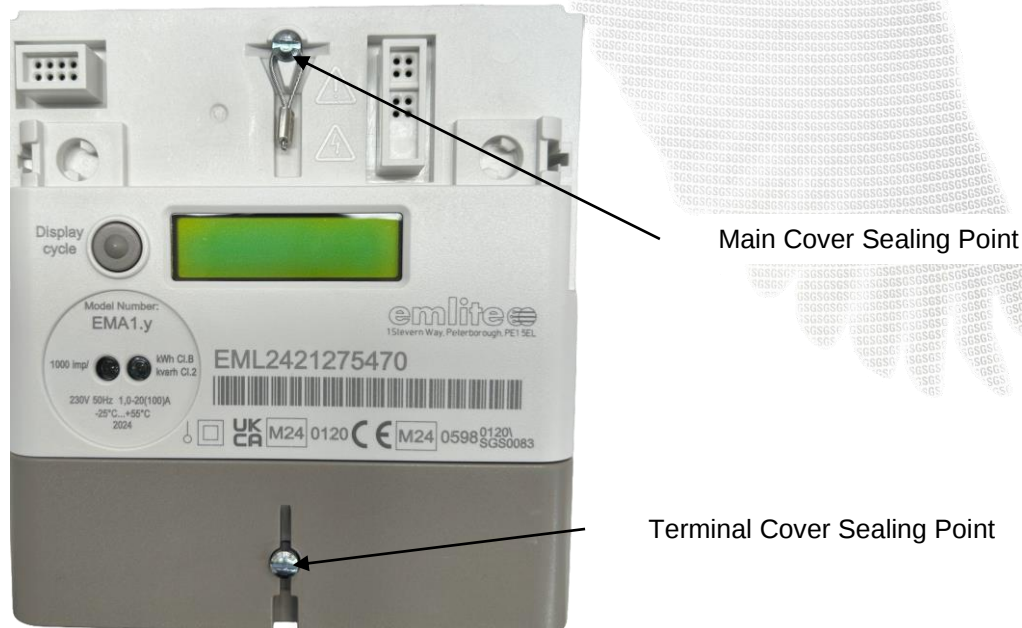

	EU-Type Examination Certificate Number:	
	0120/SGS0083/R1	
	Issue Number: 2	Dated: 19 th June 2024

3. Examples of Nameplates

Display cycle

Model Number:
ECA1.*

Property of:
SGS Sample

emlite

15Istevrn Way, Peterborough, PE1 5EL

1000 imp/

KWh Cl.B

EML2425123456

230V 50Hz 0,25-5(100)A
-40°C...+70°C
2024

UK

CA

M24

0120

CE

M24

0598

0120\

SGS0083

Display cycle

Model Number:
EMA1.*

Property of:
SGS Sample

emlite

15Istevrn Way, Peterborough, PE1 5EL

1000 imp/

KWh Cl.B
kvarh Cl.2

EML2425123456

230V 50Hz 0,25-5(100)A
-40°C...+70°C
2024

UK

CA

M24

0120

CE

M24

0598

0120\

SGS0083

Display cycle

Model Number:
EMB1.*

Property of:
SGS Sample

emlite

15Istevrn Way, Peterborough, PE1 5EL

1000 imp/

KWh Cl.B
kvarh Cl.2

EML2425123456

230V 50Hz 0,25-5(100)A
-40°C...+70°C
2024

UK

CA

M24

0120

CE

M24

0598

0120\

SGS0083

Display cycle

Model Number:
EMC1.*

Property of:
SGS Sample

emlite

15Istevrn Way, Peterborough, PE1 5EL

1000 imp/

KWh Cl.B
kvarh Cl.2

EML2425123456

230V 50Hz 2x0,25-5(100)A
-40°C...+70°C
2024

UK

CA

M24

0120

CE

M24

0598

0120\

SGS0083

	EU-Type Examination Certificate Number:	
	0120/SGS0083/R1	
	Issue Number: 2	Dated: 19 th June 2024

4. Calculation of the composite error/ MPE

During the type approval examination the influence factors for temperature, frequency and voltage are determined per load point. The table below represents the sum of the square values per load, determined via the following formula:-

$$\delta e(T, U, f) = \sqrt{(\delta e^2(T, I, \cos\phi) + \delta e^2(U, I, \cos\phi) + \delta e^2(f, I, \cos\phi))}$$

where

$\delta e(T, I, \cos\phi)$	=	Additional error due to variation of the temperature at the same load
$\delta e(U, I, \cos\phi)$	=	Additional error due to variation of the voltage at the same load
$\delta e(f, I, \cos\phi)$	=	Additional error due to variation of the frequency at the same load

		Influence Factors for Temperature, Voltage & Frequency							
Current	PF Cos	-40°C	-25°C	-10°C	5°C	30°C	40°C	55°C	70°C
I _{min}	1.0	0.30	0.42	0.29	0.15	0.10	0.16	0.36	0.39
I _{tr}	1.0	0.41	0.46	0.33	0.20	0.05	0.13	0.28	0.45
10I _{tr}	1.0	0.23	0.11	0.03	0.04	0.14	0.17	0.24	0.33
I _{max}	1.0	0.28	0.09	0.09	0.14	0.25	0.27	0.37	0.25
I _{tr}	0.5ind	0.31	0.48	0.39	0.29	0.17	0.14	0.20	0.24
10I _{tr}	0.5ind	0.25	0.05	0.06	0.09	0.17	0.20	0.23	0.25
I _{max}	0.5ind	0.27	0.19	0.26	0.32	0.41	0.44	0.53	0.12
I _{tr}	0.8cap	0.57	0.64	0.50	0.37	0.16	0.15	0.27	0.44
10I _{tr}	0.8cap	0.24	0.15	0.06	0.04	0.13	0.16	0.24	0.38
I _{max}	0.8cap	0.27	0.07	0.10	0.17	0.30	0.33	0.43	0.28

	EU-Type Examination Certificate Number:	
	0120/SGS0083/R1	
	Issue Number: 2	Dated: 19 th June 2024

5. Annex of Variants

Product Variant Identification Details:

Type Designation	Description of meter
ECA1.z	4 terminal basic variant, no auxiliary connections, no modular comms, no breaker
ECA1.y	4 terminal with auxiliary relay, no modular comms, no breaker
EMA1.z	4 terminal basic variant, no auxiliary connections
EMA1.az	4 terminal basic variant, no auxiliary connections, no breaker
EMA1.y	4 terminal with auxiliary relay
EMA1.ay	4 terminal with auxiliary relay, no breaker
EMA1.x	4 terminal with external hub connections
EMA1.w	4 terminal with auxiliary relay and external hub connections
EMB1.z	5 terminal (100A Heating Control) basic variant, no auxiliary connections
EMB1.y	5 terminal with auxiliary relay
EMB1.ay	5 terminal (100A Heating Control) with auxiliary relay, no breaker
EMB1.x	5 terminal with external hub connections
EMB1.w	5 terminal with auxiliary relay and external hub connections
EMC1.z	Twin element basic variant, no auxiliary connections
EMC1.az	Twin element basic variant, no auxiliary connections, no breakers
EMC1.y	Twin element with auxiliary relay
EMC1.ay	Twin element basic variant, with auxiliary relay, breaker on element 2
EMC1.x	Twin element with external hub connections
EMC1.w	Twin element with auxiliary relay and external hub connections
EMC1.w	Twin element with auxiliary relay and external hub connections
EMC1.by	Twin element basic variant, with auxiliary relay, breaker on element 1
EMC1.cz	Twin element basic variant, with 25A relay and breaker on element 2
MC11	Smart module and gateway for use with all variants

Modifications to the meter(s) described according to approval No. **0120/SGS0083** must be notified to the issuing body to confirm the meter(s) continuing compliance to the relevant pattern approval standard(s).

	EU-Type Examination Certificate Number:	
	0120/SGS0083/R1	
	Issue Number: 2	Dated: 19 th June 2024

6. Document Revision History

Issue	Date	Comments
1	23/03/2020	Initial Issue
2	19/06/2024	Alternative voltage regulator (as per latest BOM) due to supply issues. Change of LED (as per latest BOM) due to supply issues. Minor PCB modification New BOM versions for EMA1.*, EMB1.* and EMC1.* variants New meter photos

This document is issued by the Company subject to its General Conditions for Certification Services, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.

Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 28 days only.

END OF CERTIFICATE